Validation of Temperature Measurements from the Airborne Raman Ozone Temperature and Aerosol Lidar During SOLVE

John Burris, Thomas McGee and Walter Hoegy
Laboratory for Atmospheres, Goddard Space Flight Center, Greenbelt, Md. 20771

Leslie Lait, Laurence Twigg and Grant Sumnicht
Science Systems and Applications, Inc. 5900 Princess Garden Parkway, Lanham, Md. 20706

William Heaps
The Instrument Technology Center, Goddard Space Flight Center, Greenbelt, Md. 20771

Chris Hostetler
Radiation and Aerosols Branch, Mail Stop 435, Langley Research Center, Hampton, Va. 23681-2199

T. Paul Bui
Mail Stop 245-5, Ames Research Center, Moffett Field, Ca. 94035

Roland Neuber
Alfred Wegner Institute for Polar Research, Telegrafenberg A43, D-14473 Potsdam, Germany

I. Stuart McDermid
Table Mountain Facility, Jet Propulsion Laboratory, Wrightwood, Ca. 92397

Abstract. The Airborne Raman Ozone, Temperature and Aerosol Lidar (AROTEL) participated in the recent Sage III Ozone Loss and Validation Experiment (SOLVE) by providing profiles of aerosols, polar stratospheric clouds (PSCs), ozone and temperature with high vertical and horizontal resolution. Temperatures were derived from just above the aircraft to ~60 kilometers geometric altitude with a reported vertical resolution of between 0.5 and 1.5 km. The horizontal footprint varied from 4 to 70 km. This paper explores the measurement uncertainties associated with the temperature retrievals and makes comparisons with independent, coincident, measurements of temperature. Measurement uncertainties range from 0.1K to ~4K depending on altitude and integration time. Comparisons between AROTEL and balloon sonde temperatures retrieved under clear sky conditions using both Rayleigh and Raman scattered data showed AROTEL ~1 K colder than sonde values. Comparisons between AROTEL and the Meteorological Measurement System (MMS) on NASA's ER-2 show AROTEL being from 2-3 K colder for altitudes ranging from 14 to 18 km. Temperature comparisons between AROTEL and the United Kingdom Meteorological Office's model showed differences of approximately 1 K below ~25 km and a very strong cold bias of ~12 K at altitudes between 30 and 35 km.

Introduction

NASA Goddard Space Flight Center's Airborne Raman, Ozone, Temperature and Aerosol Lidar (AROTEL) participated in the SAGE III Ozone Loss and Validation Experiment (SOLVE) campaign during the winter of 1999/2000. This campaign, conducted jointly with the Third European Stratospheric Experiment on Ozone (THESEO), was based in Kiruna, Sweden and combined measurements from ground, balloon, aircraft and space-based platforms to study the processes governing ozone loss within the polar stratosphere. A second goal of the SOLVE campaign was to have been the validation of data products from the SAGE III instrument had it been launched. A key measurement for both satellite validation and ozone loss was temperature. Temperature plays a critical role in determining both the extent and duration of polar stratospheric clouds (PSCs) on whose surfaces inactive reservoir species are converted to reactive species that destroy ozone. Lidar temperature retrievals from an aircraft platform provide a unique data set that is acquired simultaneously with other onboard measurements. Retrievals can be made at times and locations inaccessible to a satellite instrument thereby affording a more comprehensive picture of atmospheric phenomena. AROTEL temperature retrievals offered significantly better vertical and horizontal resolution than was possible with a satellite instrument; the horizontal footprint can be varied between 4 and 70 kilometers while the reported vertical resolution extends from 500 to 1500 meters depending on altitude and integration time. In this paper we will present comparisons between AROTEL temperatures and those derived from coincident balloon sondes measurements. Comparisons between AROTEL temperatures and those retrieved by the Meteorological Measurement System (MMS) on the ER-2 will be made for dates on which the DC-8 and ER-2 flew coincident tracks. A study of temperature differences between AROTEL and those derived from the United Kingdom Meteorological Office (UKMO), National Centers for Environmental Prediction (NCEP) and NASA Goddard Space Flight Center's Data Assimilation Office (DAO) models will be made.

Instrument and Technique

AROTEL is a Rayleigh/Raman lidar that utilizes a hardware configuration previously validated on other Goddard Space Flight Center lidars. Temperature data was acquired using a laser operating at a wavelength of 355 nm. This wavelength permitted the use of strong Rayleigh and Raman UV backscattering while avoiding signal attenuation from the temperature dependent Huggins ozone band. Photon counting was utilized for data acquisition because of its large dynamic range and sensitivity to low signal levels. Photomultiplier tubes (PMTs), pulse height discriminators and multi-channel scalar cards constituted the detection system and were employed for all channels. Wavelength discrimination was provided by bandpass filters with ~1 nm bandpass and high transmission. Filters enabled the design of a compact detector with high detection efficiency but restricted temperature retrievals to solar zenith angles (SZAs) > 95 degrees. A complete discussion of the AROTEL instrument is provided in *McGee et al.* [this issue]. AROTEL's operational characteristics relevant to the temperature measurement are provided in Table 1.

AROTEL temperatures were retrieved using an algorithm proven in numerous previous field campaigns, a discussion of issues relating to the temperature retrieval is covered in *Gross et al.* [1997]. Temperatures were derived from data created by both elastic (Rayleigh) molecular scattering and inelastic (Raman) scattering by molecular nitrogen. These data are directly proportional to atmospheric number density. Temperatures are calculated using relative, not absolute, number densities thus making the retrieval insensitive to many instrumental parameters such as telescope size, photomultiplier tube quantum efficiency and detector transmission efficiency. Elastic scattering, with returns ~2000 times more intense than those from inelastic backscattering, provided numerous advantages such as more distant ranging, enhanced vertical resolution, better signal to noise and more rapid data acquisition. The sensitivity of elastic molecular scattering to interference by Mie scattering from aerosols, thin cirrus and PSCs, however, limited its use to altitudes above 20-25 km (unless otherwise noted all altitudes are geometric). Because of the wavelength shift associated with inelastic scattering (~2331cm^{-1} for N$_2$), it is, to first order, not affected by Mie scattering from clouds and aerosols. Reported inelastic temperature retrievals extend from the aircraft

to ~25 km altitude, elastic retrievals are reported to ~45 km. Besides temperature, AROTEL provided several additional data products including ozone profiles to ~30 km and both backscatter and extinction data for aerosols at 355 nm. NASA's Langley Research Center (LaRC)used data derived from scattering at 532 and 1064 nm to calculate aerosol backscattering and extinction coefficients and depolarization ratios (532 nm). These data were acquired simultaneously with the AROTEL aerosol (UV), ozone and temperature retrievals.

Table 1. AROTEL Instrument

Wavelength(nm)	355	387
Energy/pulse	200 millijoules	
Repetition rate	50 Hz	
Receiver diameter	40 cm	
Effective area (cm^2)	~1240	
Altitude range (km)	12-60	12-25
Data bin size(meters)	150	150
Horizontal resolution	4.0 - 70 km	
Vertical resolution	0.5 - 1.5 km	
Precision	<1-4 K	<1-5 K

Measurement Uncertainties

Temperature uncertainties, in the absence of optically thick clouds and aerosols, are influenced by several mechanisms. Below ~40 km, statistical errors inherent in photon counting are the most important. These errors depend critically upon whether elastic or inelastic returns are used because of the marked differences in scattering cross section between the two processes. Rayleigh scattering of both the laser pulse and return signal can cause significant signal loss for both elastic and inelastic data, a correction is applied to all data. Since the instrument actually measures the local atmospheric density profile this correction is made using the retrieved density. Signals are also impacted by the desired vertical and horizontal resolution, the range between aircraft and scattering volume and how the signal is partitioned between the various detectors. The large dynamic range in returns from just above the aircraft to beyond 60 km altitude requires splitting the return signals among multiple PMTs. Intense returns can introduce non-linearities in the PMT's background count rate that make it difficult to ascertain the true count rate for low signal levels. These non-linearities were minimized by gating (effectively setting the PMT gain to zero while the outward propagating laser pulse is still close to the lidar). Extremely high count rates also affect signal linearity because of discriminator saturation, a correction to convert observed into actual counts was made. Except in the presence of optically thick clouds, extremely high count rates were generally not an issue because all PMTs were operated in a regime where the background counts remained linear.

Additional noise sources included dark counts associated with the PMTs (minimal) and counts that, depending upon operational conditions, originated with the sun or moon and fell within the detector's bandpass. Aurora were observed on several occasions but their emission was outside the instrument's detection bandpass. For temperature retrievals the full capability of the instrument was realized for solar zenith angles (SZA) ≥95 degrees, however, temperatures were derived for SZAs as low as 85 degrees. As the SZA decreased, the increased solar background restricted the maximum altitude of the measurement and significantly impacted the measurement uncertainty due to the high background count rates.

The retrieval algorithm must be initialized and this introduces a uncertainty above ~40 km. Temperatures were calculated using a routine initialized at the maximum altitude of the retrieval, typically

between 54 and 60 km. Initialization was accomplished utilizing either a model (CIRA86) or temperature profile calculated using data from the Data Assimilation Office at Goddard Space Flight Center for the aircraft's projected flight track. Errors using DAO temperatures at the 0.5 mbar pressure level are ≤5 K (Steve Pawson - private communication). At 40 km the impact of the DAO tie-on uncertainty is < 0.7 K and at 30 km it falls below 0.1 K. Using a model to tie-on at 60 km can introduce larger uncertainties since it is based upon the general climatology. The CIRA86 model provided temperatures, pressures and densities from 0 to 120 km in 5 km intervals based on both monthly and zonal averages. CIRA86 and DAO generally differed by less than 10 K at the tie on altitude, this introduced an error in the retrieved temperatures at 35 km of < 0.5 K.

In addition to clear air, temperatures can be retrieved above optically thin clouds and aerosols, however, the additional signal attenuation increases reported errors. Temperatures can occasionally be derived above optically thick clouds depending on signal levels. Temperature retrievals within optically thick PSCs or aerosol layers are not considered here because of the inability to adequately correct for Mie scattering and signal attenuation. Neither can they be derived below optically thick clouds. Retrievals within clouds are made using inelastic scattering. A detailed discussion of temperature profiling within optically thin clouds and aerosol layers will be discussed in an upcoming paper currently in preparation.

Measurement uncertainties as a function of altitude for both the Rayleigh and Raman temperatures are given in Figure 1.

AROTEL and Balloon Sonde Temperatures

During SOLVE, the DC-8 made numerous overflights of the Network to Detect Stratospheric Change (NDSC) site at Ny Ålesund, on Spitsbergen island, as part of a correlative measurements effort. Balloon sondes were launched to coincide with DC-8 overflights of the island and thereby provide ozone and temperature profiles from within the same volume sampled by AROTEL. Other sonde sites used for validation included two sites on Greenland's east coast (Danmarkshavn and Scoresbvsund), Iceland (Keflavik) and two Norwegian (Jan Mayen and Bjornoya Island) sites. Several issues developed in using sondes as part of a correlative measurement effort. The first arose because sonde observations were not always coincident the DC-8's flight track, either in time or space. For the comparisons reported here the maximum horizontal distance between the DC-8 and sonde launch site was less than or equal to 100 km, the largest separation in time between the sonde and DC-8's closest approach was ~11 hours. Lidar temperatures within ±150 meters of a reported sonde altitude were averaged together for the comparison. The second issue concerned the relatively low bursting altitude of the meteorological sondes, 20 to 25 km, which prevented the acquisition of a good data set within the 25-35 km region. Figure 2 presents a plot of sonde versus lidar temperatures for flight date December 7, 1999.

Mean differences between AROTEL and all balloon sonde temperature data used in the comparison as a function of altitude are given in terms of elastic and inelastically derived temperatures in Figures 3 and 4. Reported uncertainties in sonde temperatures at 100 mbar (~15 km) are ≤0.5 K, ~1 K at 20 mbar (~26 km) and ~4 K at 10 mbar (~30 km) [Schmidlin, 1988]. Sonde temperatures are reported over altitude intervals ranging from ~10 to ~1000 meters. For temperatures derived from elastically scattered returns, the AROTEL minus sonde difference was -1.1 ± 0.6 K between 12 and 28 km. The mean difference for inelastically determined temperature was -1.2 ± 1.1 K between 12 and 26 km altitude. No systematic differences were found between the lidar and sonde temperature measurements as a function of the sonde's distance from closest approach to the aircraft's flight track and for time differences of up to 11 hours (the maximum difference).

AROTEL and MMS Temperature Comparison

Several opportunities for correlative measurements with the ER-2's MMS became available during SOLVE. MMS provides a number of data products including pressure, horizontal and vertical winds and in-situ temperature at the ER-2's flight altitude [Scott et al., 1990]. Temperatures are derived from a resistive

measurement on an open platinum wire calibrated against a NIST standard. Corrections to the static temperature were made for thermodynamic heating as a function of the aircraft's MACH number. On January 20, 2000 both the DC-8 and ER-2 followed essentially the same flight track from Kiruna towards the North Pole and back again. The criteria employed to define coincidence on this flight required the measurement sites differ by no more than 30 km horizontally and be separated by less than 10 minutes in time. This test provided numerous coincidence pairs between ~14.5 km and 18 km geometric altitude. Since PSCs were observed by the co-located LaRC aerosol lidar during significant portions of the flight, inelastic temperatures were utilized because of their relative insensitivity to optically thin PSCs and aerosols. The data indicated that AROTEL had a cold bias of approximately 2.5 ± 0.9 K compared to reported MMS temperatures (Figure 5). AROTEL temperatures were calculated using a 5 minute data set and had reported errors ranging from ~0.4 to 1.0K over this altitude range; the effective vertical resolution was ~0.5 km. MMS has a reported precision of 0.3K, an accuracy of 0.2% (~0.4K for this altitude) and one second resolution. On both January 27, 2000 and March 5, 2000 additional comparisons were made between MMS and AROTEL temperatures retrieved employing both elastic and inelastic returns. The criteria for coincidence used here was 30 km horizontally and ≤5 hours in time. Inelastic data for January 27[th] had a mean difference between AROTEL and MMS of -2.8 ± 0.5 K while the March 5[th] flight demonstrated a mean difference of -1.9 ± 0.2 K. Temperatures calculated using elastic returns also displayed a cold bias with respect to MMS of -2.0±1.8 K for January 27[th], for March 5[th] a bias of -2.6±0.8 K was observed. All measurements demonstrated that both the inelastic and elastically derived AROTEL temperatures were from 2 to 3 K colder than reported MMS values.

Ny Ålesund and Mauna Loa Temperatures: Lidar and Sondes

As a result of the observed cold temperature biases in AROTEL temperatures when compared against both MMS and the balloon sondes a study was undertaken of temperatures retrieved by Goddard's STROZ-LITE Ozone and Temperature lidar during two previous field campaigns. This is a mobile system installed inside a trailer with a 39" telescope, a xenon chloride excimer laser operating at 308 nm and a xenon fluoride excimer at 351 nm. Temperature data is derived from elastically scattered data at 351nm and inelastically scattered returns at 382 nm [McGee et al., 1995]. The close physical similarity between the STROZ-LITE and AROTEL lidars and the utilization of a similar temperature algorithm by both instruments suggested a study utilizing STROZ-LITE's more extensive data base could help identity the origin of these biases. The data sets chosen included a winter campaign at the Arctic NDSC site on Spitsbergen Island, Ny Ålesund, during 1998 and a summer campaign at a site on Mauna Loa in Hawaii during 1995. Specific questions were whether biases had been observed in the data during these two campaigns and, if so, what were their magnitude and sign. An additional opportunity for an independent correlative study was provided by Stuart McDermid's JPL lidar also located on Mauna Loa during the same 1995 campaign [McDermid et al., 1991].

The Ny Ålesund study consisted of ten dates in January and February of 1998 during which correlative measurements were made. A total of 1373 separate temperature differences were calculated. Lidar retrievals began at ~10 km with a reported altitude resolution of from 1 to 3 km depending on altitude. Reported uncertainties ranged from 0.1 to 0.5 K for data sets acquired with ~60 minutes of data. Data retrieved in the presence of PSCs was not used in the comparison. The comparison showed that the lidar temperatures had a small cold bias relative to the sondes of ~-1.4±1.9 K over altitudes between 15 to ~32 km (Figure 6).

A second correlative measurements opportunity involved the NDSC intercomparison campaign on the island of Hawaii during August and September, 1995. Numerous temperature retrievals were made by STROZ-LITE and compared to balloon sondes, another ground-based lidar (McDermid) and National Meteorological Center (NMC) values. Balloon sondes were launched from Hilo, Hawaii and timed to coincide with data acquisition by the lidars. As with the Ny Ålesund data, the Mauna Loa intercomparison showed that the STROZ-LITE lidar exhibited a slight cold bias relative to the sondes (Figure 7). A total of 16 dates were employed and the resulting biases ranged from ~0 K at 15 km to ~-4 K at 30 km. The reported altitude resolution varied with altitude from 1 to 3 km; measurement uncertainties ranged from ~0.1 K at 15 km to

~0.5 K at 30 km for approximately 90 minutes of data. Another temperature and ozone lidar on Mauna Loa, operated by Stuart McDermid of JPL, also provided temperature profiles available for comparison with balloon sonde profiles during 1995. An identical analysis was performed for the same time frame as above using data reported by McDermid and again a slight cold bias was observed in the lidar temperatures relative to the sondes (see figure 8). This bias ranged from ~2.1 K at 15 km to ~0 at 20 km and ~-2 K at 35 km. The reported altitude resolution varied between 1 and 6 km. Reported measurement uncertainties as a function of altitude were between 0.2 K and 1 K.

These results suggest that temperatures derived from lidar data have a small but real cold bias when compared to temperatures retrieved by balloon sondes regardless of whether the data was acquired in the tropics or Arctic. The differences observed from these ground-based measurements are consistent with those observed by AROTEL during the SOLVE campaign (-1.2±1.1 K for inelastically derived temperatures, -1.1±0.6 K for temperatures derived from elastically scatter data).

Model Temperatures

A correlative study was carried out using AROTEL temperatures and those calculated by three global gridded meteorological analyses: the NASA Goddard Space Flight Center's Data Assimilation Office (DAO) product, the United Kingdom Meteorological Office (UKMO) product generated for the Upper Atmosphere Research Satellite (UARS) project, and data reanalysis generated by National Centers for Environmental Prediction (NCEP) and the National Center for Atmospheric Research (NCAR). All three are generated by data assimilation procedures in which satellite, rawindsonde, and other measurements are merged into a running model so that the resulting data are consistent with both the measurements and atmospheric physics.

The DAO fields for the SOLVE period are obtained from the GEOS-3 assimilation system for EOS-Terra support. GEOS-3 is the successor to the GEOS-1 system documented in Pfaendtner et al. [1995]. These data grids lie on 36 pressure levels ranging from 1000 hPa to 0.2 hPa, have a horizontal resolution of one degree longitude by one degree latitude, and are produced at 0000, 0600, 1200, and 1800 UTC each day.

The UKMO UARS fields are supplemental correlative data for the UARS Project and are described in Swinbank and O'Neil [1994]. The version used here are grids which consist of 18 pressure surfaces from 1000 hPa to 0.4 hPa, have a horizontal resolution of 3.75 degrees longitude by 2.5 degrees latitude, and are produced at 1200 UTC daily.

The NCEP/NCAR reanalysis system's procedures are applied consistently to over 40 years of raw data, resulting in a dataset which is useful for long-term studies. (For further information, see Kalney et al., 1996). These data consist of 17 pressure surfaces from 1000 hPa to 10 hPa, have a horizontal resolution of 2.5 degrees longitude by 2.5 degrees latitude, and are produced at 0000, 0600, 1200, and 1800 UTC daily.

Differences between lidar and model were calculated for temperatures retrieved using elastic and inelastic returns on all flight dates for which data was reported. Temperature retrievals employing elastic backscatter within PSCs were excluded as were retrievals using inelastic data within or below optically thick clouds. The flights on December 7, 1999 and December 12[th] were representative of dates during which PSCs were and were not observed by the co-located LaRC lidar. Differences were calculated for all three models and are qualitatively similar however we present only the UKMO results here. Between flight altitude (10-12 km) and ~25 km the mean difference between AROTEL inelastic temperatures and UKMO temperatures for December 7, 1999 was 0.7± 1.9 K, for December 12, 1999 AROTEL was slightly colder: -1.0 ± 1.3 K (Figures 9 and 10). Elastically derived temperatures to ~40 km for December 7 were marginally colder than the models, -2.4±4.4 K; for December 12, AROTEL was again slightly colder, -2.8±4.2 K. Elastically derived temperatures between 32 and 33 km altitude repeatedly showed large cold biases with respect to the models (Figures 11 and 12). For December 7[th] the mean difference between AROTEL and UKMO at 32.8 km was -12.6±1.4 K. The December 12[th] differences were -12.3±2.2 K at 32.6 km. When these altitudes are removed from the calculation the mean difference between AROTEL and UKMO for December 7[th] was -0.6±1.3 K, for December 12[th] it was -1.2±1.6 K which are consistent with differences

derived for the inelastically derived temperatures.

The large differences between AROTEL and model temperatures in the region of from ~30 and 35 km were surprising given the much small differences observed between AROTEL and both MMS and balloon sonde temperatures. As was previously done for the sonde measurements, data sets acquired by the STROZ-LITE lidar during deployments to both polar and tropical sites were used for comparisons with model forecast made from ~10 km to over 50 km altitude. To provide a consistent model temperature product for previously acquired data only results from the UKMO model were used for these comparison. Data from the Arctic site at Ny Ålesund provided temperatures on 17 dates between January 20, 1998 and February 9 1998. Differences between STROZ-LITE and UMKO were calculated between 10 and ~40 km altitude (Figure 13). The mean difference between STROZ-LITE and UKMO was -1.1±8.8 K for altitudes from 10.8 to 38.7 km. There was a slight cold bias of ~1 K from 10 to 22 km which increased to over 9 K at 32.6 km. Reported temperature errors for these data sets range from 0.1 at 10 km to 0.3 K at 38 km with an effective vertical resolution of between 1 and 3 km.

The STROZ-LITE data set acquired at Mauna Loa in 1995 and used in the sonde comparison above was also compared to UKMO temperature profiles for the specified dates. Here, unlike Ny Ålesund, the UKMO temperatures displayed much better agreement with the lidar as shown in Figure 14. Data was acquired on 16 dates from August 15, 1995 through September 1, 1995. A slight cold bias was noted between 30 and 40 km, at 31.3 km the mean difference between lidar and UKMO was -2.0 K and at 36.1 km it was -2.7 K. Differences were calculated from 14.2 km to 55.2 km with a mean difference of -0.9 K. Calculated uncertainties ranged from ~0.1 K to ~0.6 K at 55 km. The lidar's reported vertical resolution ranged from 1km at the lower end to ~ 3 km at 30 km and, because most of the signal was directed at the high altitude channel, ~2 km at 55 km.

Temperatures derived from data acquired by the JPL lidar were also compared to those from the UKMO model. For the previously reported data set, JPL reported a slight cold bias of -0.5 K averaged over data from 14.3 to 55.4 km (Figure 15). The largest biases were noted at 36.0 km at -5.0 K. Typical errors for the JPL measurements ranged from 0.2 to 1.0 K with a reported vertical resolution of from ~1.0 to 7 km.

These results suggest that between 30 to 40 km altitude, systematic biases exist between the lidars and models. Both the JPL lidar and STROZ-LITE had, with respect to the UKMO temperatures, a slight cold bias in the tropics while STROZ-LITE and AROTEL displayed much larger temperature differences against UKMO in the polar regions; the origin of these differences in the polar region is not known but may be due to the limited number of soundings available to the modeling community within this altitude range.

Conclusions

AROTEL temperatures, retrieved during the SOLVE campaign, have been compared with those from balloon sondes and the MMS instrument onboard the ER-2. A slight cold bias was found in both comparisons; when compared to MMS the difference varied between 2-3 K while temperatures derived from balloon sondes were 1.2 ±1.1 K warmer than inelastically derived AROTEL temperatures and 1.1 ±0.6 K warmer than temperatures derived from elastically scattered data. AROTEL temperatures, when compared to several temperature models (DAO, NCEP and UKMO), showed differences that were less than or equal to 1 K below ~30 km. Between 30 - 40 km AROTEL displayed a large cold bias of 12 K against the UKMO model. Significant temperature biases at these altitudes were also observed in data acquired by another Goddard lidar, STROZ-LITE, during a winter campaign correlative measurements campaign at Ny Ålesund in 1998. These cold biases were significantly smaller in data acquired in Hawaii during a 1995 campaign. The good agreement between AROTEL and model below 30 km altitude suggest the discrepancy above 30 km is due to the limited number of retrievals available for use by the models in the polar region.

References:

Gross, M., T.J. McGee, R.A. Ferrare, U.N. Singh and P. Kimvilakani , Temperature measurements made with a combined Rayleigh-Mie and Raman lidar, *Appl. Opt.* 36, 5987-5994, 1997.

Kalnay, E., M. Kanamitsu, R. Kistler, W. Collins, D. Deaven, L. Gandin, M. Iredell, S. Saha, G. White, J. Woollen, Y. Zhu, M. Chelliah, W. Ebisuzaki, W. Higgins, J. Janowiak, K. C. Mo, C. Ropelewski, J. Wang, A. Leetmaa, R. Reynolds, R. Jenne, and D. Joseph, The NCEP/NCAR 40-year reanalysis project, Bull. Am. Met. Soc., 77, 437-471, 1996.

McDermid, I. S., D. A. Haner, M. M. Kleinman, T. D. Walsh and M. L. White, Differential Absorption Lidar Systems for Tropospheric and Stratospheric Ozone Measurements, *Opt. Eng., 30,* 22-30, 1991.

McGee, T. J., M. Gross, U. N. Singh, J. J. Butler and P. Kimvilakani, An Improved Stratospheric Ozone Lidar, *Opt. Eng., 34,* 1421-1430, 1995.

McGee, T. J., J. Burris, L. Twigg, Wm. Heaps, G. Sumnicht, W. Hoegy and C. Hostetler, AROTEL: An Airborne Ozone, Aerosol and Temperature Lidar, this issue.

Pfaendtner, J., S. Bloom, D. Lamich, M. Seablom, M. Sienkiewicz, J. Stobie, and A. da Silva, Documentation of the Goddard Earth Observing System (GEOS) Data Assimilation System - Version 1, NASA Technical Memorandum 104606, Vol. 4, 1995.

Schmidlin, F. J., Instrument and Observing Methods: WMO International Radiosonde Intercomparison Phase II, 1985, *WMO Rep. 29, WMO/TD-32,* World Meteorol. Organ., Geneva, 1988.

Scott, S. G., K. R. Chan, S. W. Bowen, and T. P. Bui, The Meteorological Measurement System on the NASA ER-2 aircraft, *J. Atmos. Oceanic Technol.,* 7, 525-540, 1990.

Swinbank, R., and A. O'Neil, A stratosphere-troposphere data assimilation system, Mon. Wea. Rev., 122, 686-702, 1994.
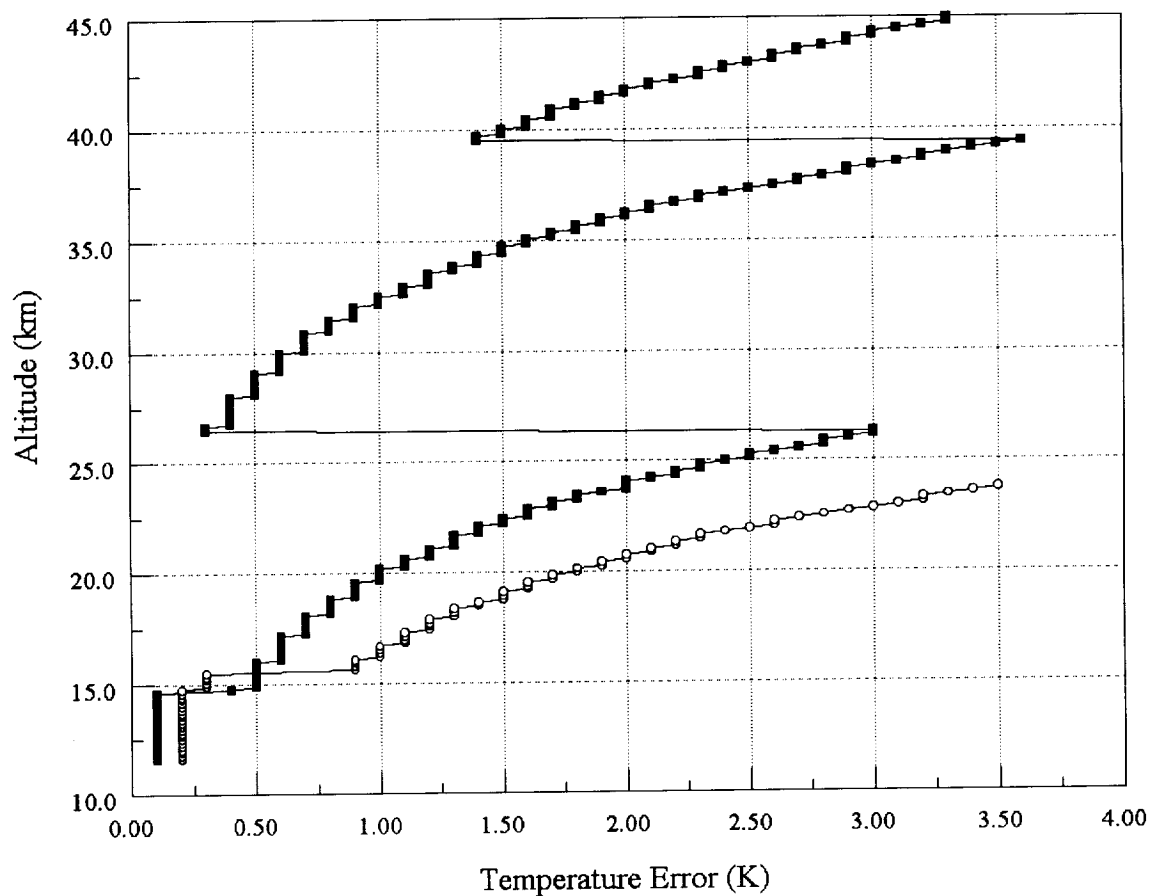
Figure Captions

Figure 1. Temperature uncertainties versus altitude for temperatures derived from elastic (Rayleigh) and inelastically (Raman) scattered data for flight date 991207. Open circles are inelastic temperature errors, solid squares are for elastically derived temperature errors.

Figure 2. Balloon sonde versus AROTEL inelastic temperatures acquired on flight date 991207 over Ny Ålesund. The sonde's maximum altitude was almost 27 km. The minimum temperature was ~190 K at 25 km in good agreement with AROTEL at 189 K.

Figure 3. AROTEL (elastic) temperatures minus all sonde temperature retrievals that occurred within 100 km and 12 hours of a DC-8 flight track. The mean difference between AROTEL and the sondes was -1.1± 0.6 K between 12 and 28 km altitude.

Figure 4. AROTEL (inelastic) temperatures minus all sonde temperature retrievals acquired within 100 km and 12 hours of a DC-8 flight track. The mean difference between lidar and sonde was -1.2 ± 1.1 K between 12 and 26 km altitude.

Figure 5. AROTEL (inelastic) - MMS temperature differences for flight date 000120. Coincidences were for MMS retrievals made within 30 km and 10 minutes of the DC-8 flight track. The mean difference was -2.5 ± 0.9 K.

Figure 6. STROZ-LITE minus balloon sonde temperatures for Ny Ålesund deployment in 1998. The mean difference was -1.4 ± 1.9 K between 15 and 30 km.

Figure 7. STROZ-LITE minus balloon sonde temperatures for Mauna Loa campaign in 1995. The mean temperature difference was -1.5 ± 2.0 K. At 15 km the difference was +0.5 ± 1.3 K; at 20 km, -1.5 ± 1.0 K; at 25 km, -1.9 ± 0.7 K; at 30 km, -4.0 ± 1.4 K and at 35 km the difference was -0.2 ± 1.3 K.

Figure 8. JPL - sonde temperatures for Mauna Loa campaign in 1995. The computed mean difference was 0.0 ± 1.7 K.

Figure 9. Temperature difference plot of AROTEL minus UKMO for December 7, 1999. AROTEL temperatures were derived using inelastically scattered data. The mean difference was -0.7±1.9 K.

Figure 10. Temperature difference plot of AROTEL minus UKMO for December 12, 1999. AROTEL temperatures were derived using inelastically scattered data. The mean difference was -1.0±1.3 K.

Figure 11. Temperature difference plot of AROTEL minus UKMO for December 7, 1999. AROTEL temperatures were derived using elastically scattered data. The mean difference was -2.4±4.4 K. The mean difference at 32.8 km was -12.6±1.4 K. Removing the value at 32.8 km results in a mean difference between AROTEL and UKMO of -0.6±1.3 K.

Figure 12. Temperature difference plot of AROTEL minus UKMO for December 12, 1999. AROTEL temperatures were derived using elastically scattered data. The mean difference was -2.8±4.2 K. The mean difference at 32.6 km was -12.3±2.2 K. Calculating the temperature difference without including the large perturbation at 32. 6 km gives a value of -1.2±1.6 K.

Figure 13. STROZ-LITE minus UKMO model temperatures at Ny Ålesund during the 1998 NDSC campaign. Differences between STROZ-LITE and UMKO were calculated between 10 and

~40 km altitude. The mean difference between STROZ-LITE and UKMO was -2.7±4.2 K for altitudes from 10 to 40 km. There was a slight cold bias of ~1 K from 10 to 22 km which increased to over 9 K at 32.6 km. Reported temperature errors for these data sets range from 0.1 at 10 km to 0.3 K at 38 km with an effective vertical resolution of between 1 and 3 km.

Figure 14.   STROZ-LITE minus UKMO model temperatures during the Mauna Loa NDSC correlative measurements campaign in 1995. Data was acquired on 16 dates from August 15[th] through September 1[st], 1995. A slight cold bias was noted between 30 and 40 km, at 31.3 km the mean difference between lidar and UKMO was -2.0 ± 2.5 K and at 36.1 km it was -2.8 ± 2.2 K. Differences were calculated from 14.2 km to 55.2 km with a mean difference of -0.9 ± 2.7 K. Calculated uncertainties ranged from ~0.1 K to ~0.6 K at 55 km. The lidar's resolution ranged from 1km at the lower end to ~ 3 km at 30 km and back to 2 km at 55 km.

Figure 15.   JPL - UKMO model temperatures during the Mauna Loa NDSC campaign in 1995. The JPL data had a slight cold bias of -0.5 ± 3.0 K averaged between 14.3 and 55.4 km altitude. The largest bias was noted at 36.0 km at -5.0 ± 1.8 K. Typical errors for the JPL measurements ranged from 0.2 to 1.0 K with a reported vertical resolution of from ~1.0 to 7 km.

Figure 1   Temperature uncertainties versus altitude for temperatures derived from elastic (Rayleigh) and inelastically (Raman) scattered data for flight 991207. Open circles are inelastic temperature errors, solid squares are for elastically derived temperature errors.
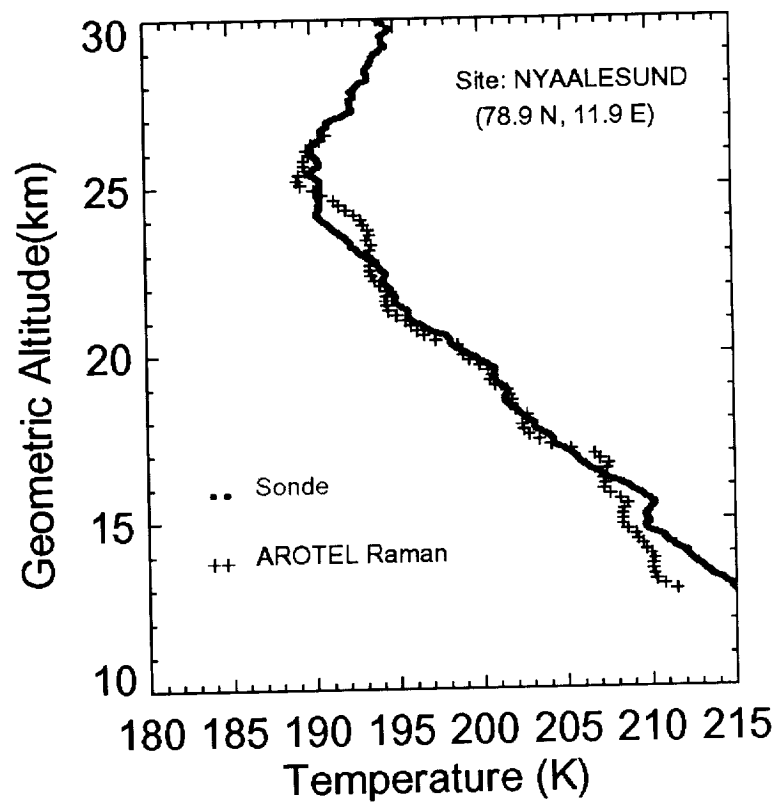
7 December, 1999

Site: NYAALESUND
(78.9 N, 11.9 E)

• • Sonde

+ + AROTEL Raman

Figure 2   Balloon sonde versus AROTEL inelastic temperatures acquired on flight date 991207 over Ny Ålesund. The sonde's maximum altitude was almost 27 km. The minimum temperature was ~190 K which was in good agreement with AROTEL at ~189 K.
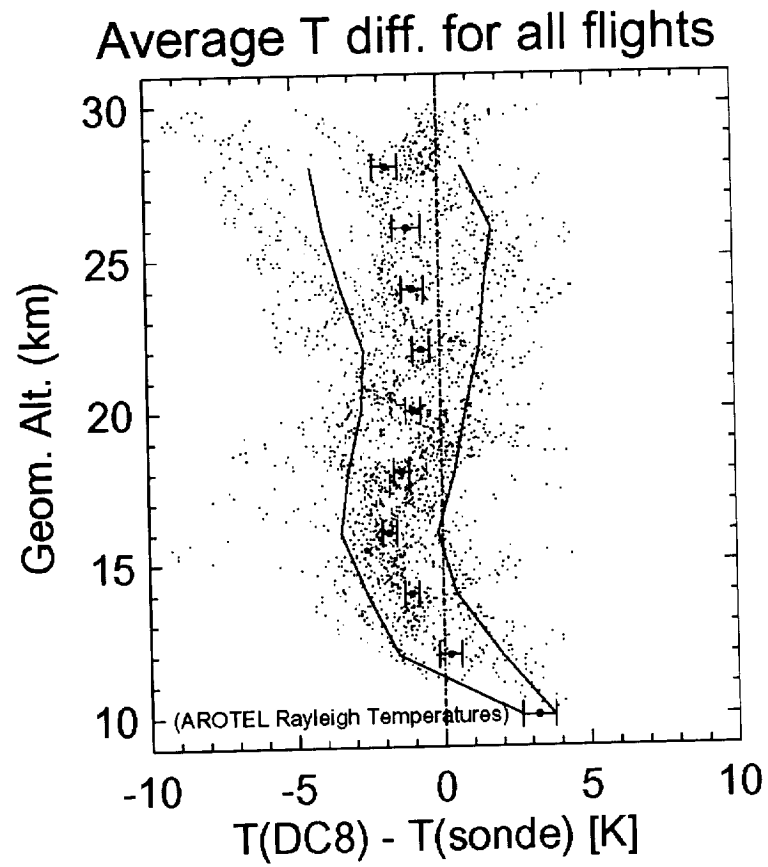
Average T diff. for all flights

Geom. Alt. (km) vs. T(DC8) - T(sonde) [K]

(AROTEL Rayleigh Temperatures)

Figure 3 AROTEL (elastic) temperatures minus all sonde temperature retrievals that occurred within 100 km and 12 hours of a DC-8 flight track. The mean difference between AROTEL and the sondes was -1.1±0.6 K between 10 and 28 km.
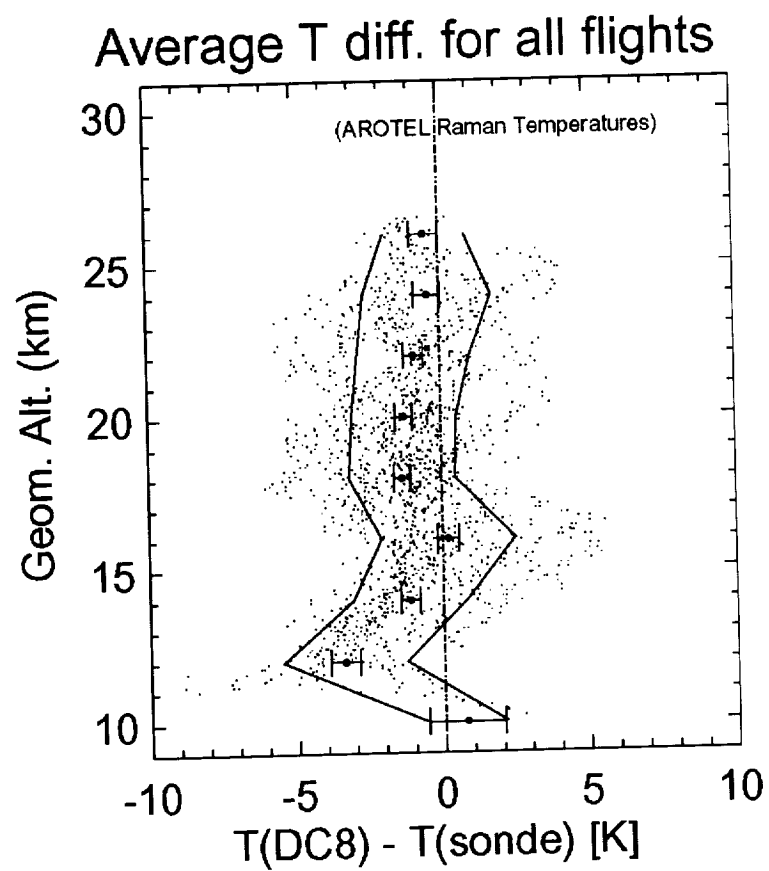
Figure 4   AROTEL (inelastic) temperatures minus all sonde temperature retrievals acquired within 100 km and 12 hours of a DC-8 flight track. The mean difference between AROTEL and sonde was -1.0±1.1 K between 12 and 26 km.
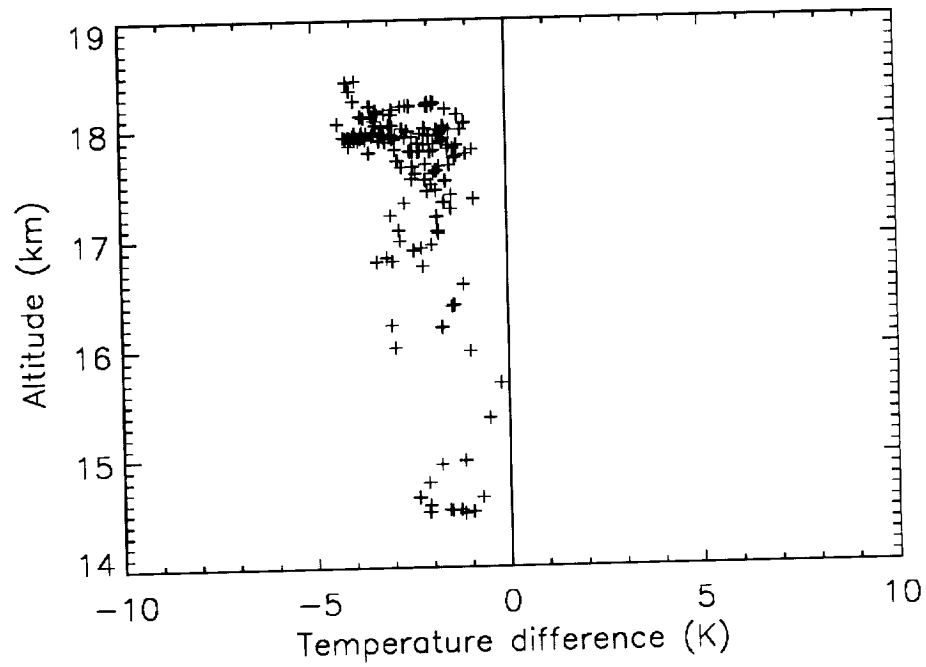
Figure 5   AROTEL (inelastic) - MMS temperature differences for flight date 000120. Coincidences were for MMS retrievals made within 30 km and 10 minutes of the DC-8 flight track. The mean difference was -2.5±0.9 K.
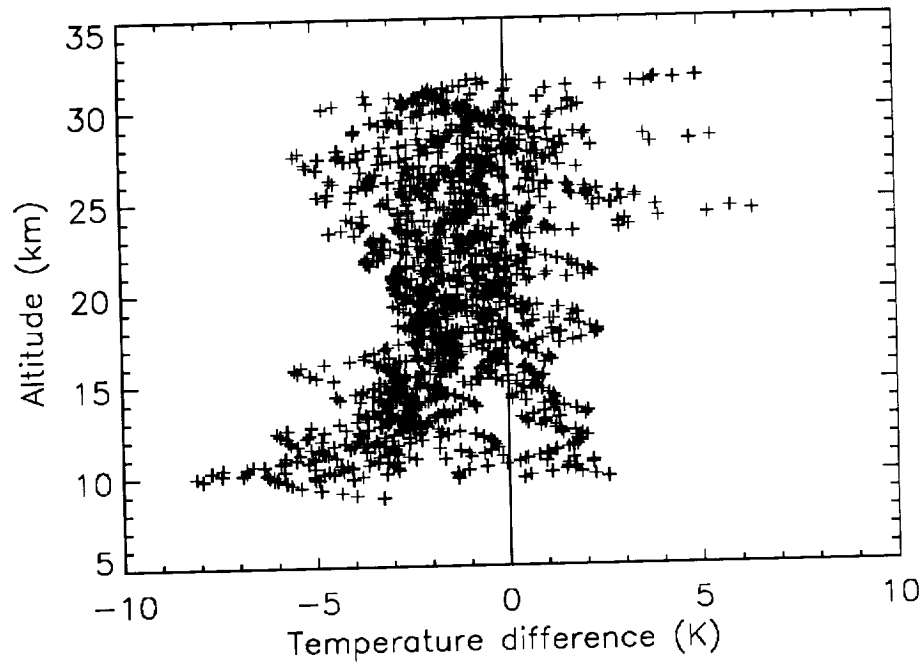
Figure 6 STROZ-LITE minus balloon sonde temperatures for the Ny Ålesund deployment in 1998. The mean difference was -1.4±1.9 K between 15 and 30 km.
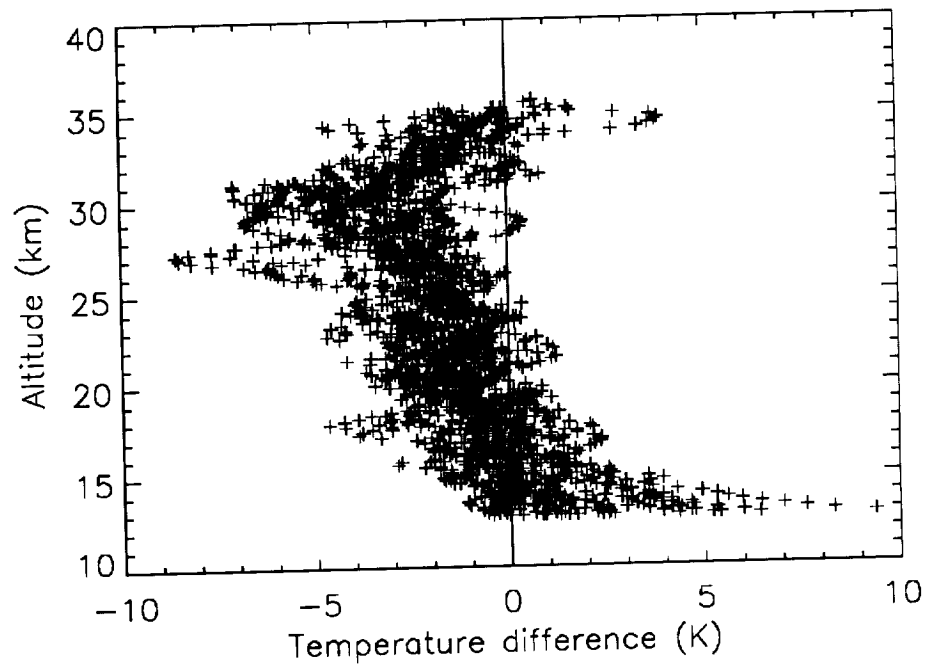
Figure 7 STROZ-LITE minus balloon sonde temperatures for the Mauna Loa campaign in 1995. The mean temperature difference was -1.5±2.0 K. At 15 km the difference was +0.5±1.3 K; at 20 km, -1.5±1.0 K; at 25 km, -1.9±0.7 K; at 30 km, -4.0±1.4K and at 35 km -0.2±1.3 K.
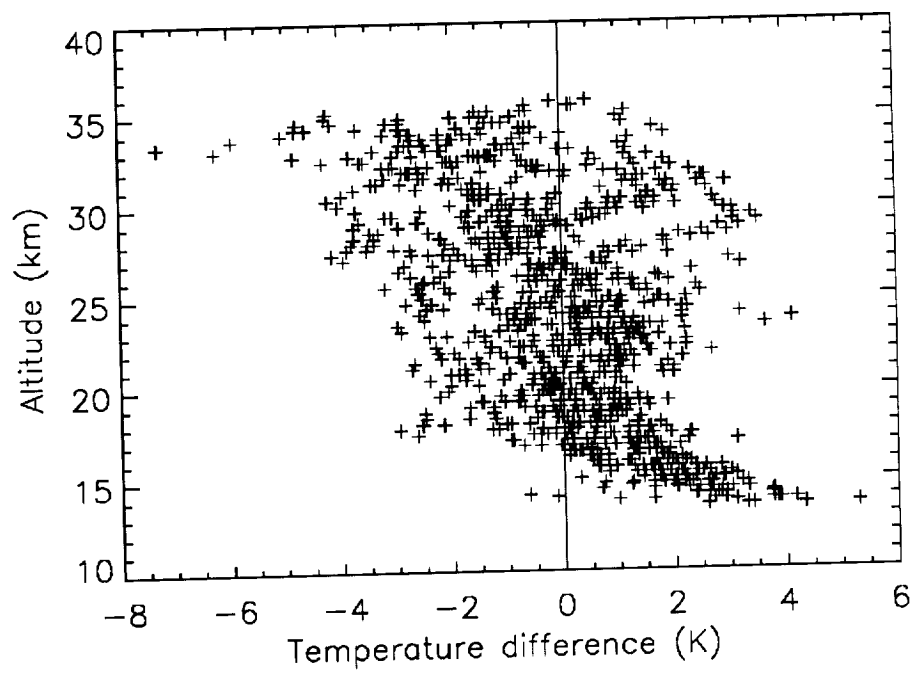
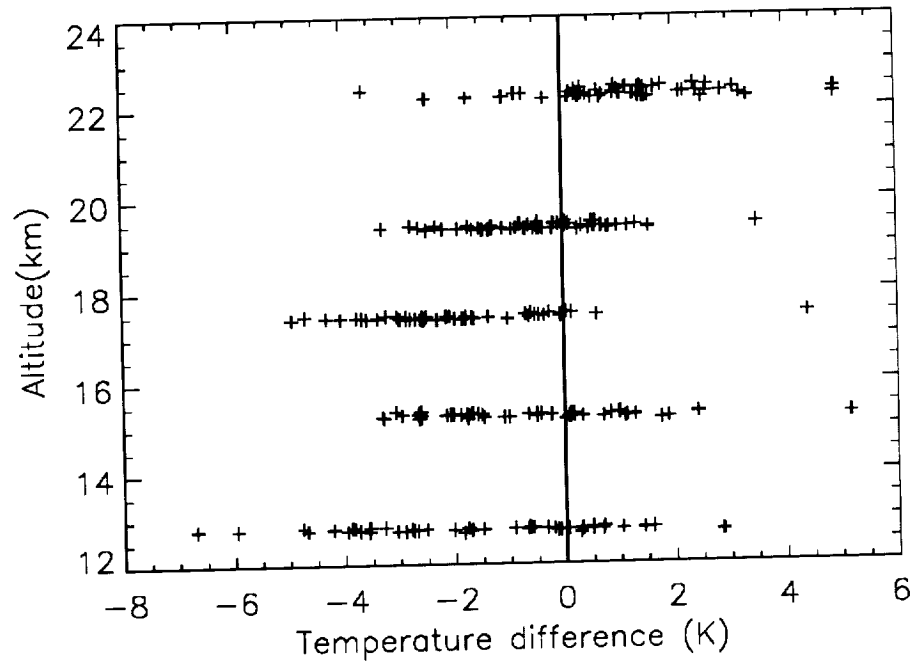**Figure 8**   JPL - sonde temperatures for Mauna Loa campaign in 1995. The computed mean difference was 0.0±1.7 K.

Figure 9   Temperature difference plot of AROTEL minus UKMO for December 7, 1999. AROTEL temperatures were derived using inelastically scattered data. The mean difference was -0.7±1.9 K.
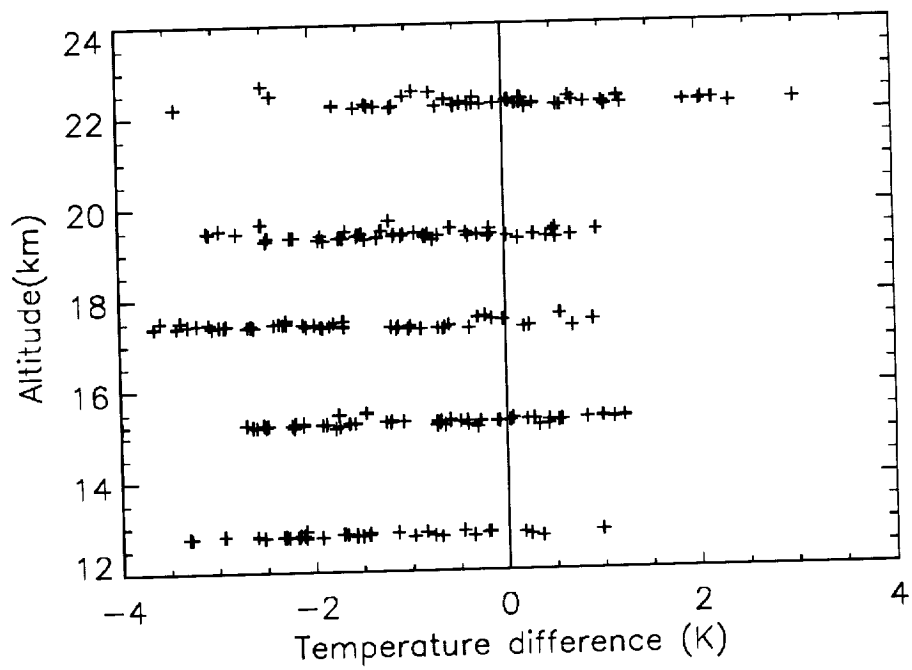
Figure 10   Temperature difference plot of AROTEL minus UKMO for December 12, 1999. AROTEL temperatures were derived using inelastically scattered data. The mean difference was -1.0±1.3 K.
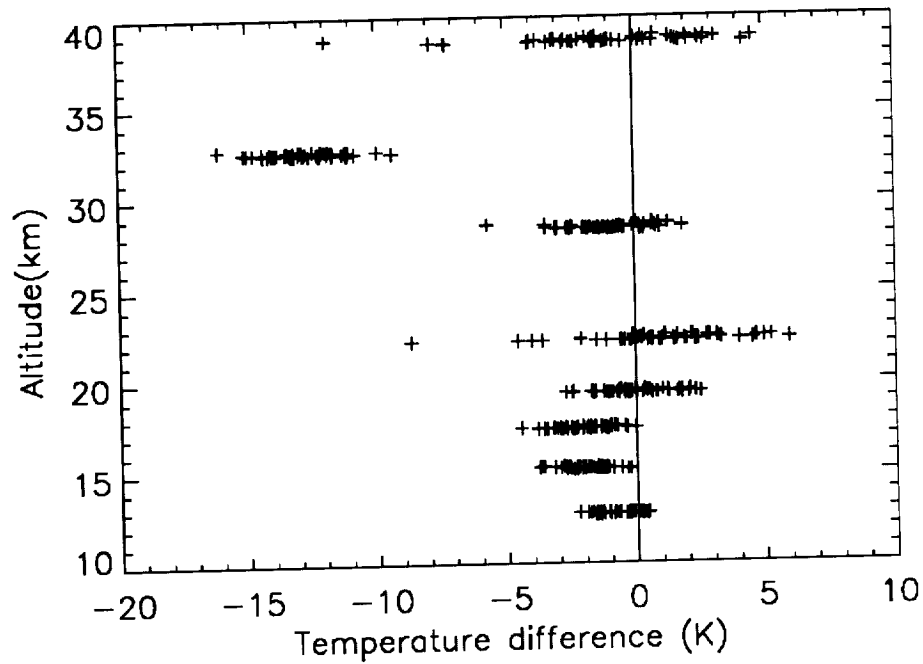
Figure 11 Temperature difference plot of AROTEL minus UKMO for December 7, 1999. AROTEL temperatures were derived using elastically scattered data. The mean difference was -2.4±4.4 K. The mean difference at 32.8 km was -12.6±1.4 K. Removing the value at 32.8 km results in a mean difference between AROTEL and UKMO of -0.6±1.3 K.
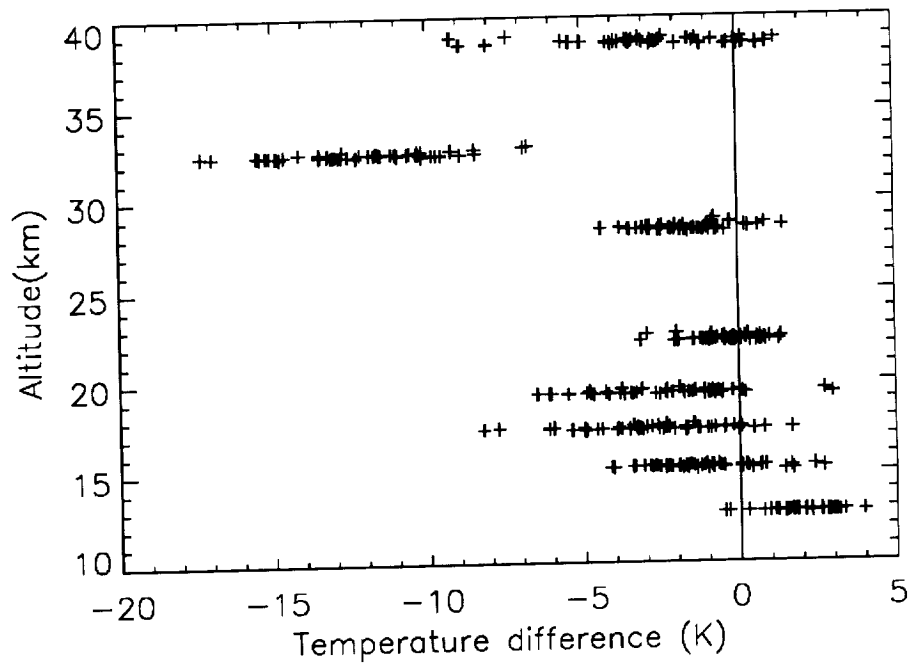
Figure 12   Temperature difference plot of AROTEL minus UKMO for December 12, 1999. AROTEL temperatures were derived using elastically scattered data. The mean difference was -2.8±4.2 K. The mean difference at 32.6 km was -12.3±2.2 K. Calculating the temperature difference without including the large perturbation at 32. 6 km gives a value of -1.2±1.6 K.
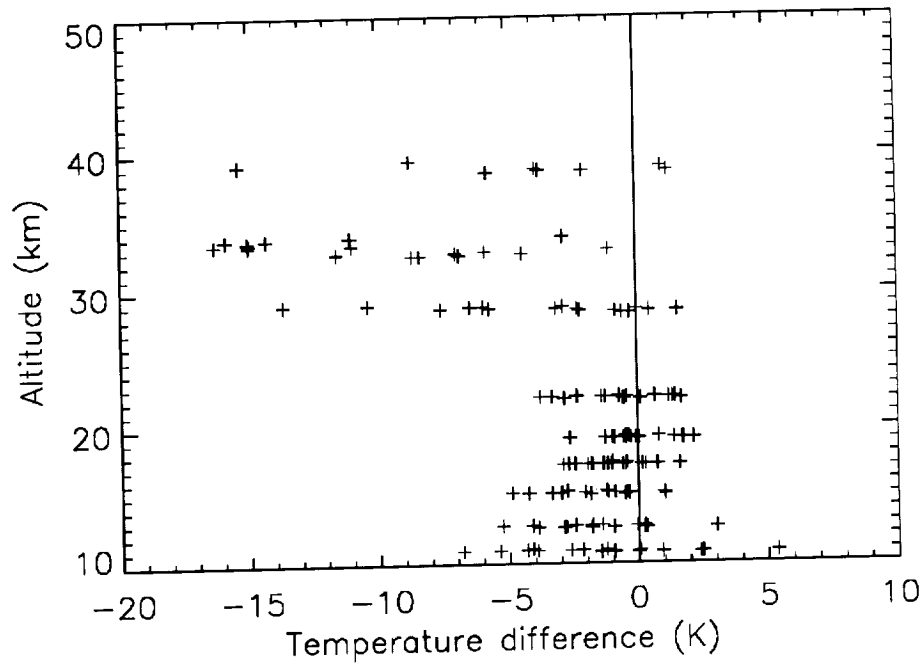
Figure 13   STROZ-LITE minus UKMO model temperatures at Ny Ålesund during the 1998 NDSC campaign. Differences between STROZ-LITE and UKMO were calculated between 10 and ~40 km altitude. The mean difference was -2.7±4.2 K. There was a slight cold bias of ~1K from 10 to 22 km which increased to over 9 K at 32.6 km. Reported temperature errors for these data sets range from 0.1 K at 10 km to 0.3 K at 38 km with an effective vertical resolution of between 1 and 3 km.
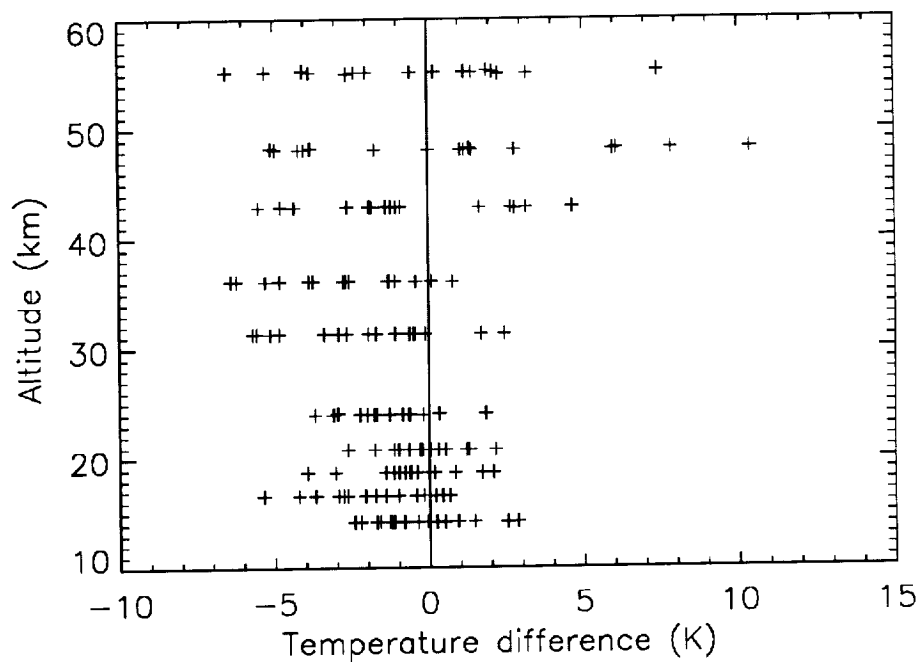
Figure 14   STROZ-LITE minus UKMO model temperatures during the Mauna Loa NDSC correlative measurements campaign in 1995. Data was acquired on 16 dates from August 15[th] through September 1[st]. A slight cold bias was noted between 30 and 40 km, at 31.3 km the mean difference between lidar and UKMO was -2.0 ± 2.5 K and at 36.1 km it was -2.8 ± 2.2 K. Differences were calculated from 14.2 to 55.2 km with a mean difference of -0.9 ± 2.7 K. Calculated uncertainties ranged from ~0.1 K to ~0.6 K at 55 km. The lidar's resolution ranged from 1 km at 14 km to ~3 km at 30 km and ~2 km at 55 km.
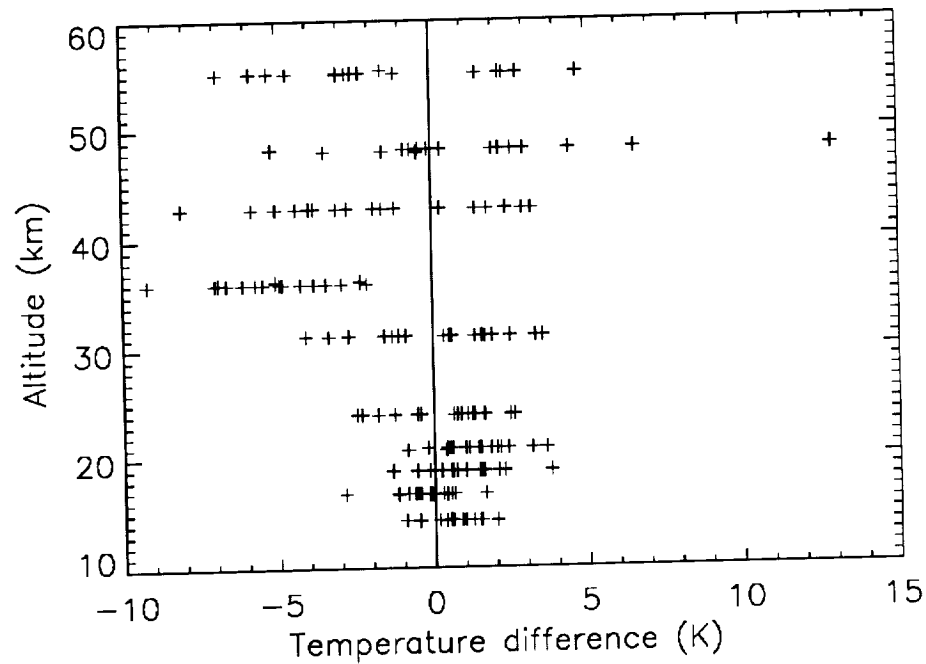
Figure 15   JPL - UKMO model temperatures during the Mauna Loa NDSC campaign in 1995. The JPL data had a slight cold bias of -0.5 ± 3.0 K averaged between 14.3 and 55.4 km altitude. The largest bias, -5.0 ± 1.8 K, was observed at 36.0 km. Typical errors for the JPL measurements ranged from 0.2 to 1.0 K with a reported vertical resolution of from ~1.0 to 7 km.

NASA Scientific and Technical Document Availability Authorization (DAA)

National Aeronautics and Space Administration

The DAA approval process applies to all forms of published NASA Scientific and Technical Information (STI), whether disseminated in print or electronically. It is to be initiated by the responsible NASA Project Officer, Technical Monitor, author or other appropriate NASA official for all presentations, reports, papers, and proceedings that contain NASA STI Explanations are on the back of this form and are presented in greater detail in NPG 2200.2, "Guidelines for Documentation, Approval, and Dissemination of NASA Scientific andTechnical Information.

☒ Original
☐ Modified

I. DOCUMENT/PROJECT IDENTIFICATION

TITLE

Validation of Temperature Measurements from the Airborne Raman Ozone Temperature and Aerosol Lidar During SOLVE

AUTHOR (S)

J. Burris, T. McGee, W. Hoegy, L. Lait, L. Twigg, G. Sumnicht, W. Heaps, T P. Bui, R. Neuber, J. S. McDermid

ORIGINATING NASA ORGANIZATION

NASA Goddard Space Flight Center

PERFORMING ORGANIZATION (if different)

Atmospheric Chemistry & Dynamics Branch

CONTRACT/GRANT/INTERAGENCY/PROJECT NUMBER(S)	DOCUMENT NUMBER(S)	DOCUMENT DATE

For presentations, documents, or other STI to be externally published (including through electronic media), enter appropriate information on the intended publication such as name, place, and date of conference, periodical or journal name, or book title and publisher in the next box. These documents must be routed to the NASA Headquarters or Center Export Control Administrator for Approval (see Sections III and VIII).

▶ **J. Geophys. Res.**

II. SECURITY CLASSIFICATION

CHECK ONE (One of the five boxes denoting Security Classification must be checked.)

☐ SECRET ☐ SECRET RD ☐ CONFIDENTIAL ☐ CONFIDENTIAL RD ☒ UNCLASSIFIED

III. AVAILABILITY CATEGORY

☐ ITAR ☐ EAR

Export Controlled Document - USML Category Classification Number (ECCN) /CCL Export Control (Documents marked in this block must have the concurrence/approval of the NASA Headquarters or Export Control Administrator (see Section VIII).

☐ TRADE SECRET
☐ SBIR
☐ COPYRIGHTED

Confidential Commercial Document (check appropriate box at left and indicate below the appropriate limitation and expiration:

☐ U.S. Goverment agencies and U.S. Government agency contractors only
☐ NASA contractors and U.S. Government only
☐ U.S. Government agencies only
☐ NASA personnel and NASA contractors only
☐ NASA personnel only
☐ Available only with the approval of issuing office
☐ Limited until (date)

☒ PUBLICLY AVAILABLE

Publicly available documents must be unclassified, may not be export controlled, may not contain trade secret or confidential commercial data, and should have cleared any applicable patents application process.

IV. DOCUMENT DISCLOSING AN INVENTION

THIS DOCUMENT MAY BE RELEASED ON (date)	NASA HQ OR CENTER PATENT OR INTELLECTUAL PROPERTY COUNSEL SIGNATURE	DATE

V. BLANKET RELEASE (OPTIONAL)

☐ All documents issued under the following contract/grant/project number may be processed as checked in Sections II and III.

☐ The blanket release authorization granted on (date)

☐ is RESCINDED - Future documents must have individual availability authorizations.

☐ is MODIFIED - Limitations for all documents processed in the STI system under the blanket release should be changed to conform to blocks as checked in Sections II and III.

GSFC STI PUBLIC DISCLOSURE EXPORT CONTROL CHECKLIST

The Export Control Office requests your assistance in assuring that your proposed disclosure of NASA scientific and technical information (STI) complies with the Export Administration Regulations (EAR, 15 CFR 730-774) and the International Traffic In Arms Regulations (ITAR, 22 CFR 120-130). The NASA Export Control Program requires that every domestic and international presentation/publication of GSFC STI be reviewed through the GSFC Export Control Office in accordance with the NASA Form 1676 NASA Scientific and Technical Document Availability Authorization (DAA) process. Release of NASA information into a public forum may provide countries with interests adverse to the United States with access to NASA technology. Failure to comply with the ITAR regulations and/or the Commerce Department regulations may subject you to fines of up to $1 million and/or up to ten years imprisonment per violation. Completion of this checklist should minimize delays in approving most requests for presentation/publication of NASA STI.

Generally, the export of information pertaining to the design, development, production, manufacture, assembly, operation, repair, testing, maintenance or modification of defense articles, *i.e.*, space flight hardware, ground tracking systems, launch vehicles to include sounding rockets and meteorological rockets, radiation hardened hardware and associated hardware and engineering units for these items are controlled by the State Department under the ITAR. A complete listing of items covered by the ITAR can be accessed at http://gsfc-bluenun.gsfc.nasa. gov/export/regsitar.htm. The export of information with respect to ground based sensors, detectors, high-speed computers, and national security and missile technology items are controlled by the U.S. Commerce Department under the EAR. If the information intended for release falls within the above categories but otherwise fits into one or more of the following exemptions, the information may be released.

EXEMPTION I
If your information is already in the public domain **in it's entirety** through a non-NASA medium and/or through NASA release previously approved by the Export Control Office, the information is exempt from further review. If the information falls into this category, you may attest that you are using this exemption by signing below.

_____, _____
Signature   Date

EXEMPTION II
If your information pertains exclusively to the release of scientific data, *i.e.* data pertaining to studies of clouds, soil, vegetation, oceans, and planets, without the disclosure of information pertaining to articles controlled by the ITAR or EAR, such as flight instruments, high speed computers, or launch vehicles, the information is exempt from further review. If the information falls into this category, you may attest that you are using this exemption by signing below.

_____, ____5/29/01____
Signature   Date

EXEMPTION III
If your information falls into the areas of concern as referenced above, but is offered at a general purpose or high level, *i.e.* poster briefs and overviews, where no specific information pertaining to ITAR or EAR controlled items is offered, the information is exempt from further review. If the information falls into this category, you may attest that you are using this exemption by signing below.

_____, _____
Signature   Date

EXEMPTION IV

If your information is not satisfied by the 3 exemptions stated above, the information may be released using exemption 125.4(b)(13) of the ITAR. Use of this exemption is afforded only to agencies of the Federal Government and allows the release of ITAR controlled information into the public domain. But the GSFC Export Control Office has determined that use of this exemption will be allowed only after we receive assurance that such release is a responsible action. To this end, an internal guideline has been established pursuant to the use of this exemption: That the information does not offer specific insight into design, design methodology, or design processes of an identified ITAR controlled item in sufficient detail (by itself or in conjunction with other publications) to allow a potential adversary to replicate, exploit and/or defeat controlled U.S. technologies. All signatures of approval on NASA Form 1676 expressly indicate concurrence with the responsible use of Exemption IV when Exemption IV has been cited by the author. If you determine that you have met this criteria, you may attest your determination by signing below, and the GSFC Export Control Office will offer favorable consideration toward approving your presentation/publication request under this special exemption.

_____, _____
Signature   Date

If you do not satisfy the above exemptions, please contact the GSFC Export Control Office for further clarification on the releasability of your information under the ITAR or EAR.

Summary of paper designed for the general public.

Validation of Temperature Measurements from the Airborne Raman Ozone Temperature and Aerosol Lidar During SOLVE

During the winter of 1999/2000, the SAGE III Ozone Loss and Validation Experiment (SOLVE) mission took place in Kiruna, Sweden. This campaign was designed to further our understanding of how ozone is destroyed in the Arctic atmosphere at altitudes of from 45,000' to 75,000' during the winter. NASA's Goddard Space Flight Center flew a new instrument, the Airborne Raman Ozone, Temperature and Aerosol Lidar (AROTEL), on NASA's DC-8. This instrument consisted of two lasers, a telescope and electronics designed to measure aerosols/clouds, ozone and temperature to beyond 100,000' altitude. Temperatures below -117 °F were repeatedly measured. AROTEL temperatures were compared against those made at the flight altitude of NASA's ER-2, approximately 60,000', when both instruments sampled the same parcel of air. AROTEL temperatures were from 3-5 °F colder than those measured on the ER-2. When compared against temperatures measured by a temperature sonde attached to a high flying balloon, temperature differences were approximately 2 °F. These measurements were uncertain to approximately 2 °F. Comparisons between AROTEL temperatures and those made by the HALOE instrument on the UARS satellite, showed agreement to within 9 °F which is similar to previous temperature measurements made by HALOE when compared to other lidars.